

FSN Ref: 2023-04(01)  
Date: 28-April-2023

FSCA Ref: 2023-04(01)

**Urgent Field Safety Notice**  
**Mölnlycke® Barrier TUR Set**

For Attention of Theatre Manager

**Contact details of local representative (name, e-mail, telephone, address etc.)**

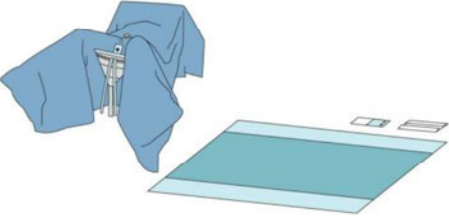
This could be a distributor or local branch of the manufacturer. To be added at the appropriate stage in the different local languages

Name: Local Customer Care contact will be added for each specific market

Email: XXX.XXX@molnlycke.com

Telephone: +XXXXXXXXXXXXXXXXX

**Urgent Field Safety Notice (FSN)**  
**Mölnlycke® Barrier TUR Set**

<b>1. Information on Affected Devices</b>	
1.	<p style="text-align: center;"><b>1. Device Type(s)</b></p> <p>Product codes: 888224-22 TUR Set Surgical drape, general/plastic surgical procedure kit, non-medicated, single-use Sterile</p> 
1.	<p style="text-align: center;"><b>2. Commercial name(s)</b></p> <p>BARRIER TUR Set</p>
1.	<p style="text-align: center;"><b>3. Primary clinical purpose of device(s)</b></p> <p>The surgical drape sets consists of both surgical drapes and supplementary products intended be used to create a sterile field for a surgical procedure.</p>
1.	<p style="text-align: center;"><b>4. Device Model/Catalogue/part number(s)</b></p> <p>See Appendix I Product Table</p>
1.	<p style="text-align: center;"><b>5. Affected serial or lot number range</b></p> <p>See Appendix I Product Table</p>


<b>2 Reason for Field Safety Corrective Action (FSCA)</b>	
2.	<p style="text-align: center;"><b>1. Description of the product problem*</b></p> <p>Mölnlycke have identified a composition error in the TUR Set. The incorrect drape has been included within the set. Drape <b><u>965520-22</u></b> has been included instead of drape <b><u>965522-22</u></b>.</p> <p>The products have different features and materials connected to the fluid pouch and therefore the dose applied to reach sterility is not high enough.</p> <p>As a precaution Mölnlycke has decided to perform a <b>Recall</b>.</p>
2.	<p style="text-align: center;"><b>2. Hazard giving rise to the FSCA*</b></p> <p>If there is a compromise in sterility of drapes which are used during a surgical procedure, there is a potential risk of a local infection.</p>

<b>3. Type of Action to mitigate the risk</b>				
<b>3.</b>	<p style="text-align: center;"><b>1. Action To Be Taken by the User</b></p> <p><input checked="" type="checkbox"/> Identify Device  <input checked="" type="checkbox"/> Quarantine Device  <input checked="" type="checkbox"/> Return Device</p> <p>We need your help in ensuring that <b><u>all affected products</u></b> are located and that below actions are performed.</p> <p>Please follow below instructions:</p> <ol style="list-style-type: none"> <li>1. <b>Identify and isolate</b> the unused Mölnlycke® BARRIER TUR Set at your facility, please see Appendix I for affected product information.</li> <li>2. Fill out the <b>Customer Reply Form</b> or <b>Distributor Reply Form</b> with quantity of identified affected products. Please sign and email/fax the <b>Customer Reply Form</b> or <b>Distributor Reply Form</b> per its instructions within 10 business days.</li> <li>3. Even if you no longer have any concerned Mölnlycke® BARRIER TUR Set, fill out the <b>Customer Reply Form</b> or <b>Distributor Reply Form</b> and return it back within 10 business days. Mölnlycke needs to be sure all customers are aware of the situation.</li> <li>4. Mölnlycke will contact you and arrange for collection of the product(s) from your facility, as soon as you return the <b>Customer Reply Form</b> or <b>Distributor Reply Form</b>. Mölnlycke will issue a credit for the goods returned.</li> <li>5. If you have forwarded any affected products to other healthcare institutions, please send them a copy of this <b>Field Safety Notice</b>. Make sure they act accordingly.</li> <li>6. If you are a distributor, please inform your customers by sending them a copy of this <b>Field Safety Notice</b>. Make sure they act accordingly and return the <b>Distributor Reply Form</b> with information collected from your end users.</li> </ol> <p>We apologize for any inconvenience this will cause you, and rest assured it is our utmost intent to make this process as easy for you as possible.</p> <p>In addition, Mölnlycke appreciates your help in collecting data on product complaints and/or incidents related to the concerned product. Please follow the reporting procedures established by your facility.</p>			
<b>3.</b>	<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td style="width: 65%;"><b>Is customer Reply Required? (If yes, form attached specifying deadline for return)</b></td> <td style="width: 30%; text-align: center;">Yes (Within 10 business days)</td> <td style="width: 5%; text-align: center;">10</td> </tr> </table>	<b>Is customer Reply Required? (If yes, form attached specifying deadline for return)</b>	Yes (Within 10 business days)	10
<b>Is customer Reply Required? (If yes, form attached specifying deadline for return)</b>	Yes (Within 10 business days)	10		

FSN Ref: 2023-04(01)

FSCA Ref: 2023-04(01)

Date: 28-April-2023

<b>4. General Information</b>		
4.	FSN Type	New
4.	Further advice or information already expected in follow-up FSN?	No
4.	1. Manufacturer information (For contact details of local representative refer to page 1 of this FSN)	
	a. Company Name	Mölnlycke Health Care AB
	b. Address	Box 130 80, SE-402 52 Gothenburg, Sweden
	c. Website address	www.molnlycke.com
4.	The Competent (Regulatory) Authority of your country has been informed about this communication to customers.	
4.	List of attachments/appendices:	Appendix I Product table Customer Reply Form
4.	Name/Signature	

<b>Transmission of this Field Safety Notice</b>	
	<p>This notice needs to be passed on all those who need to be aware within your organisation or to any organisation where the potentially affected devices have been transferred. (As appropriate)</p> <p>Please transfer this notice to other organisations on which this action has an impact. (As appropriate)</p> <p>Please maintain awareness on this notice and resulting action for an appropriate period to ensure effectiveness of the corrective action.</p> <p>Please report all device-related incidents to the manufacturer, distributor or local representative, and the national Competent Authority if appropriate, as this provides important feedback.</p>



FSN Ref: 2023-04(01)

Date: 28-April-2023

**Appendix I**

FSCA Ref: 2023-04(01)

**Product table**

<b>Material</b>	<b>Material Description</b>	<b>Batch</b>
888224-22	TUR Set	23136207

**FSN Ref:** 2023-04(01)

**FSCA Ref:** 2023-04(01)

**Date:** 26 Apr 2023

### Customer Reply Form

1. Field Safety Notice (FSN) information	
FSN Reference number	2023-04(01)
FSN Date	26 Apr 2023
Product/ Device name	See Appendix I Product table
Product Code(s)	See Appendix I Product table
Batch/Serial Number (s)	See Appendix I Product table

2. Customer Details	
Account Number	
Healthcare Organisation Name*	
Organisation Address*	
Department/Unit	
Shipping address if different to above	
Contact Name*	
Title or Function	
Telephone number*	
Email*	

3. Customer action undertaken on behalf of Healthcare Organisation					
<input type="checkbox"/>	I confirm receipt of the Field Safety Notice and that I read and understood its content. I do not have any affected devices.				
<input type="checkbox"/>	I confirm receipt of the Field Safety Notice and that I read and understood its content. I have quarantined affected devices ready for return - enter number of devices ready for return <table border="1" data-bbox="635 1384 1377 1485" style="margin-left: 20px;"> <tr> <td>Qty:</td> <td>Lot/Serial Number:</td> </tr> <tr> <td>N/A</td> <td>Comments</td> </tr> </table>	Qty:	Lot/Serial Number:	N/A	Comments
Qty:	Lot/Serial Number:				
N/A	Comments				
Print Name*					
Signature*					
Date*					

4. Return acknowledgement to sender	
Email	<a href="mailto:vigilance@molnlycke.com">vigilance@molnlycke.com</a>
Customer Helpline	+46 20-79 82 64
Postal Address	Mölnlycke Health Care, Box 130 80, SE-402 52 Gothenburg, Sweden

FSN Ref: 2023-04(01)

FSCA Ref: 2023-04(01)

Date: 26 Apr 2023

Fax	+46 31 722 34 00
Deadline for returning the customer reply form*	Within 10 days

Mandatory fields are marked with \*

It is important that your organisation takes the actions detailed in the FSN and confirms that you have received the FSN.

Your organisation's reply is the evidence we need to monitor the progress of the corrective actions.